

Certificate of Analysis

SALSA MLPA Probemix P072-D1 MSH6-MUTYH sample pictures

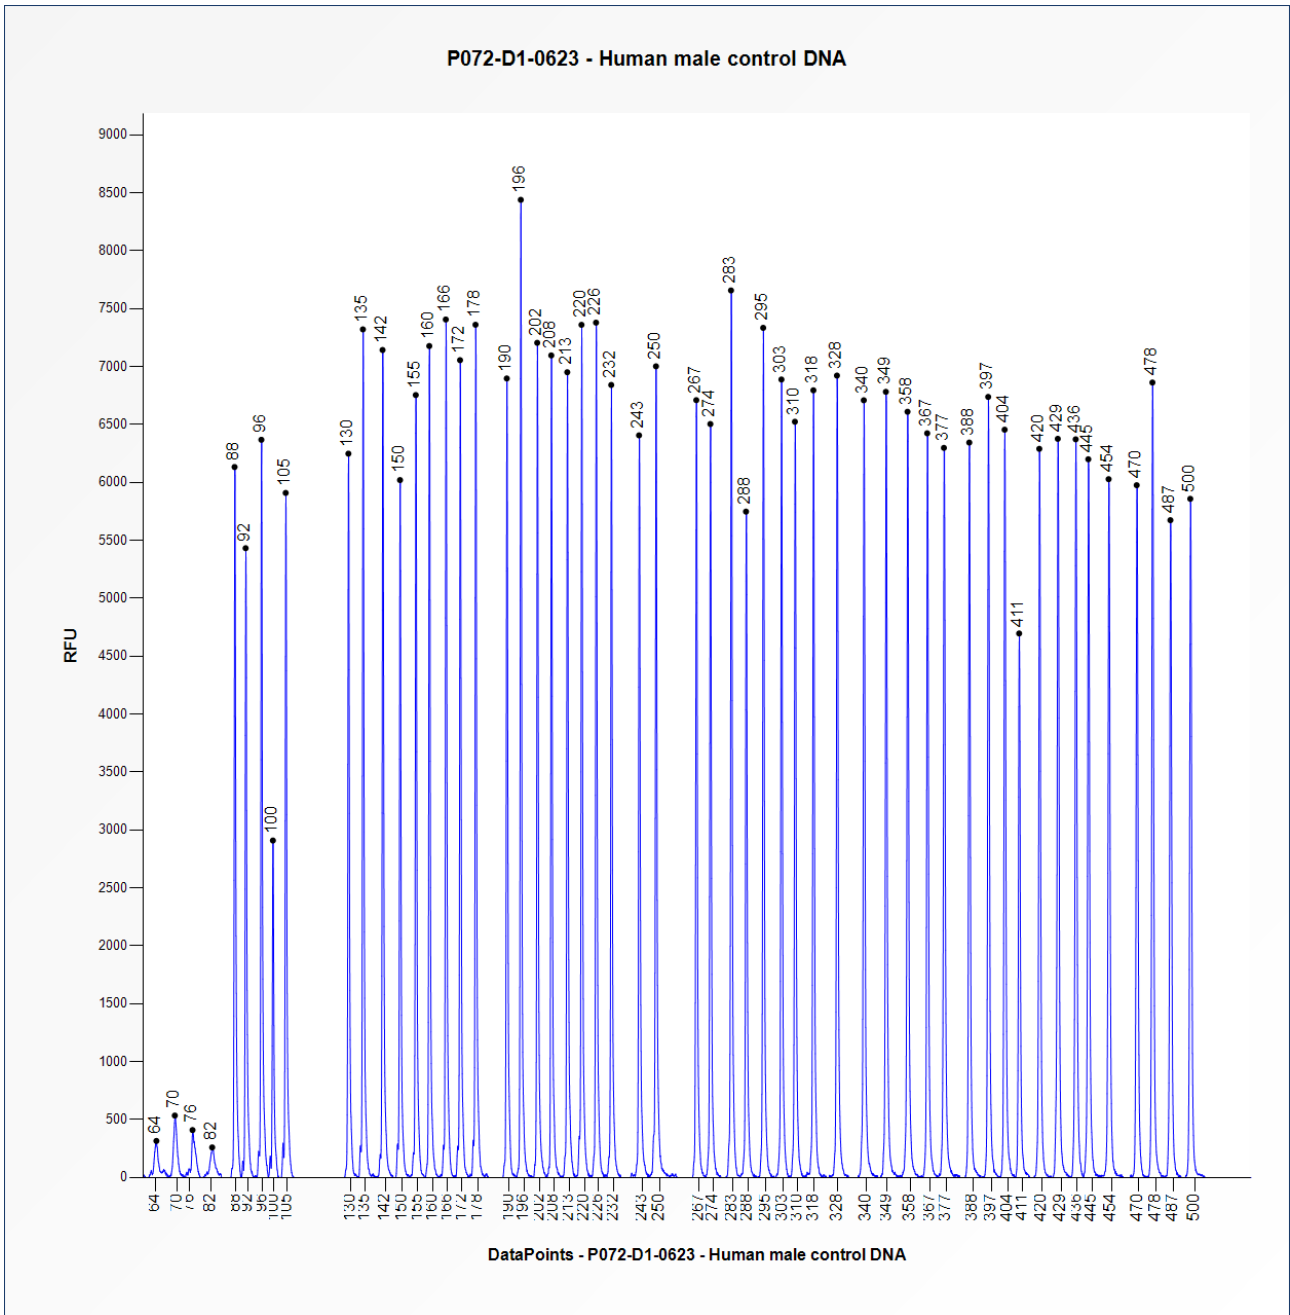


Figure 1. Capillary electrophoresis pattern from a sample of approximately 50 ng human male control DNA analysed with SALSA MLPA Probemix P072 MSH6-MUTYH (D1-0623).

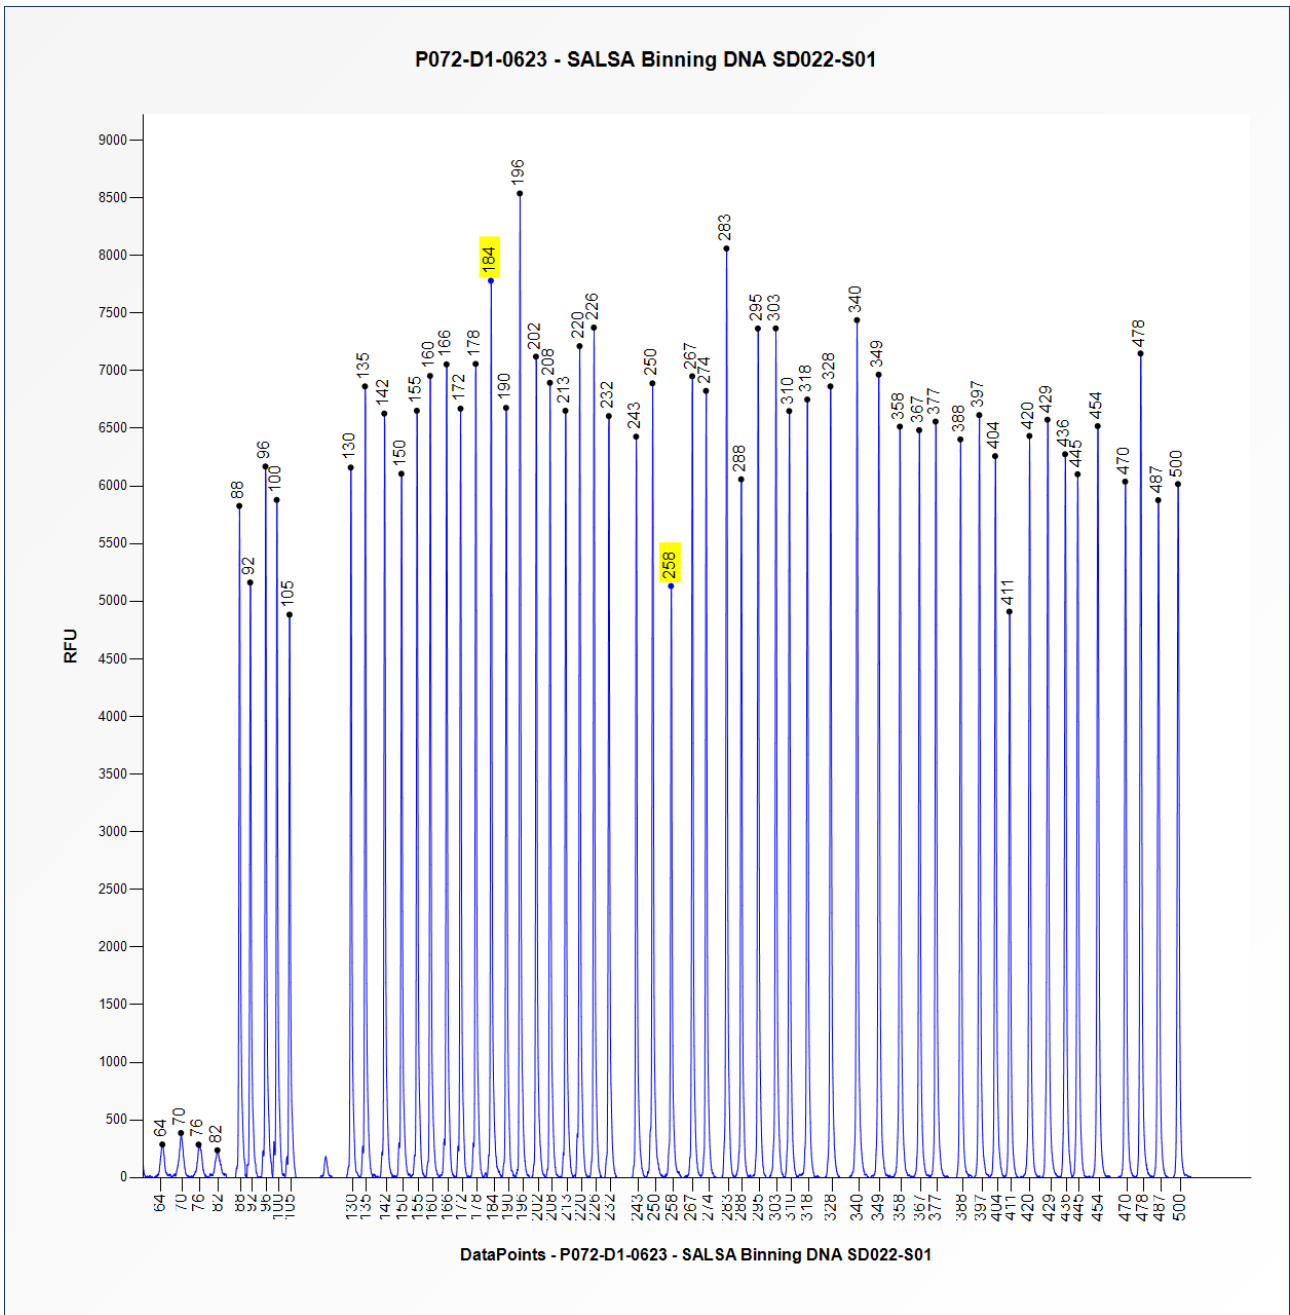


Figure 2. Capillary electrophoresis pattern from SALSA Binning DNA SD022-S01 (approximately 50 ng) analysed with SALSA MLPA Probemix P072 MSH6-MUTYH (D1-0623). The location of the *MUTYH* c.536A>G (p.Tyr179Cys) and c.1187G>A (p.Gly396Asp) mutation specific probes at 184 nt and 258 nt respectively, are indicated.

This lot was certified by MRC Holland on 19 December 2023.

This certificate is a declaration of analysis at the time of the manufacturing process. All assays were run in compliance with manufacturer’s instructions for use.

<p>Implemented changes in the COA</p> <p>Version 01 – 19 December 2023 (6) - Not applicable, new document.</p>
--